

# Restorative Handbook



# 4. Restorative Handbook

Section	Page
4.1 Neoss Implant System	4:3
4.1.1 General Features	4:3
4.1.2 Restorative Assistants	4:3
4.1.3 Esthetiline Solution	4:4
4.1.4 Neo and iGO screw overview	4:8
4.2 Impression Techniques	4:9
4.2.1 Digital impressions	4:9
4.2.2 Conventional impressions	4:13
4.3 NeoBase® and TiBase Abutments – Digital	4:16
4.3.1 NeoBase® Abutments	4:16
4.3.2 Neoss TiBase Abutments and ScanPost	4:17
4.4 NeoLink® – Gold/Titanium	4:19
4.4.1 Single Unit Construction	4:20
4.4.2 Multiple Unit Construction	4:20
4.4.3 Double Scan – Milled Constructions	4:21
4.5 Multi-Unit Abutment	4:22
4.6 Access Abutment	4:24
4.7 Provisional Abutments	4:26
4.7.1 Esthetic Tissue Formers	4:26
4.7.2 Provisional Titanium Abutments	4:27
4.8 Titanium Prepable Abutments	4:29
4.8.1 Titanium Prepable Abutment – Alternative Emergence Profiles	4:31
4.9 Zirconia Abutment	4:32
4.10 CoCr Abutment	4:34
4.11 Burnout Abutment	4:34
4.12 Overdenture Solutions	4:34
4.12.1 Ball Abutments	4:34
4.12.2 Equator Abutments	4:36

# 4.1 Neoss Implant System

The following information is a guide as requirements may vary on an individual basis.

## 4.1.1 General Features

The Neoss® Implant System provides a simple, easy to use means of anchorage for a single crown, bridge or denture thereby satisfying a wide range of aesthetic and functional requirements. Simple implant installation and flexibility in prosthetic solutions provides optimal aesthetic restorations for a wide range of clinical situations. This Handbook serve as a clinical reference for surgical and restorative assistant procedures.

### The Neoss Implant System

The Neoss Implants are based on extensive research and development, the outcome of which is a state-of-the-art system, rationalized by design. The implants have patented design and geometry which imparts specific features and benefits to the system.

Neoss implants may be used as a one or two-stage implant and are manufactured from Commercially Pure Titanium Grade IV with a surface that has been subjected to a multistage blasting, etching, cleaning and chemical treatment.. The system fulfills all clinical indications with a compact and rational range of implant components and instruments.

### The Neoss implant to abutment connection

Unique to the Neoss Implant System is the ONE prosthetic platform, across three implant ranges. The same prosthetic components fit every standard implant. All standard Neoss implants, Ø3.5 and larger, have the same standard platform (SP) with the implant to abutment connection design called Neoloc. For Ø3.25 mm implants the implant connection has a smaller narrow platform (NP).

## 4.1.2 Restorative Assistants

The principles for restoring dental implants are very similar to conventional crown and bridge techniques. Interestingly many restorative dentists and assistants find the restorative aspects of implant dentistry simpler and more rewarding than conventional crown and bridge.

The terminology used in implant dentistry is different from conventional dentistry but the treatment options are similar:

Generally the patient will present to the restorative surgery with a healing abutment in place. In the majority of cases the impression will be taken at 'Implant Level', however some abutments allow for their preparation intraorally – similar to that of a natural tooth – in these cases a conventional crown and bridge impression protocol would be followed.

*Note: Please refer to the information in this manual for procedures and information in relation to:*

- Prosthetic Tray and Instrument Kit
- Titanium Preparable Abutments
- Cleaning, Disinfection, Sterilization, Storage and Lifetime
- Zirconia Abutments
- Esthetiline Solution
- NeoLink® – Gold/Titanium
- Provisional Abutments
- Single Unit and Multiple Unit Construction
- Impression Techniques
- Overdenture Solutions
- NeoBase and TiBase Abutments
- CoCr Abutment
- Access Abutments
- Burnout Abutment

All prosthetic products and dental instruments that are delivered non-sterile must after removal of the protective transport packaging be cleaned and if required sterilized before use. This also applies for prepared abutments coming from lab.

Please see chapter 2.4 for more information.

## 4.1.3 Esthetiline Solution

The Esthetiline solution enables simple, rapid and effective anatomical tissue contouring to be developed and optimized with matching standard and individualized restorative components. The Neoss Esthetiline solution provides seamless restorative integration all the way from implant placement to final crown restoration. The natural emergence profile developed during healing is matched perfectly in permanent restorative components; Preable Titanium abutments, Zirconia abutments, custom abutments and copings, and CAD/CAM solutions as shown on next page.

Conventional Dentistry	Implant Dentistry
Tooth root	Implant
Crown preparation	Abutment
Removable dentures	Overdentures
Crown	Crown – An implant crown may be cemented onto the abutment, or screw retained to the abutment, or screw retained directly to the implant
Bridge	Bridge – A bridge may be cemented onto the abutments, or screw retained to the abutments, or screw retained directly to the implants

The gingival margin abutment profile is fixed in relation to the non-rotational feature on all Esthetiline abutments and thus related to the position of the implant – indexing. The Esthetiline solution is best applied when the implant is oriented at surgery by ensuring that there is a groove in the buccal direction. This will require the least adjustment. Indexing throughout the treatment is possible utilizing the indexing features as shown in the Esthetiline Overview on next page.

## Esthetic Healing Abutments and Tissue Formers – Healing & Provisional Abutments

Placement of Esthetic Healing Abutments and Tissue Formers at implant placement or abutment connection guides the soft tissue and enables simple creation of the optimal emergence profile. Esthetic Healing Abutments and Tissue Formers are non-rotational and made in a range of anatomical shapes which are designed to match the profiles of individual incisor, canine, pre-molar and molar teeth.

*Note: The trans-gingival section on Esthetic Healing Abutments and Tissue Formers is slightly smaller buccally than matching restorative components in order to provide additional soft tissue volume.*

*Note: The molar type can be rotated 90° if preferred but the implant has to be oriented accordingly at the time of surgery.*

### Esthetic Healing Abutments

The Esthetic Healing Abutment functions as a regular healing abutment with the purpose to create a soft tissue profile during healing. Together with the ScanPeg inserted in the Esthetic Healing Abutment, a digital impression can be recorded with an intraoral scanner. For more information about the use of Esthetic Healing Abutments please refer to section 4.2.


### Esthetic Tissue Formers

The Esthetic Tissue Formers are used for cement or screw retained provisional restorations. The titanium/polymer structure makes it highly biocompatible whilst retaining ease of preparation, strength and ability to bond to resins. For more information about the use of Esthetic Tissue Formers please refer to section "3.7 Provisional Abutments".

## Digital Impression Techniques

The ScanPeg that comes with the Esthetic Healing Abutment is a scan body momentarily fitted in the screw access hole of the Esthetic Healing Abutment to enable digital acquisition of the implant position in relation to the adjacent teeth and soft tissue.


The Esthetic Healing Abutment in combination with the ScanPeg is included in Neoss 3D libraries for design of matching CAD/CAM abutments in design software from 3shape, Exocad and Dental Wings. For more information please refer to separate instructions in section 4.2.



## Conventional Impression Techniques

There are a series of treatment options; an impression may be taken to enable laboratory fabrication of a custom abutment or gold or metal framework in a traditional manner. Preable Titanium or Zirconia abutments may also be prepared in the laboratory environment. An alternative option is to place a suitable Titanium Preable or Zirconia Abutment directly at the chair-side and take a conventional crown impression.

*Note: It may prove necessary to prepare the margins of the Titanium Preable or Zirconia Abutments, for more information please refer to sections "3.8 Titanium Preable Abutments" and "3.9 Zirconia Abutment".*



The standard Neoss impression coping is suitable for implant level impressions. There will typically be a gap between the impression coping and the sculpted anatomical gingiva which has been created by the Tissue Former. In the majority of cases the degree of tissue collapse will be minimal during the impression procedure and a normal impression technique syringing material between the coping and gingival will give an accurate result. If there is concern about tissue collapse a second Tissue Former of the same type may be used together with an impression coping screw for the impression. For more information about impression taking procedure please refer to section "3.2 Impression Techniques".

## Final restoration – CAD/CAM abutments

The Esthetic Healing Abutment in combination with the ScanPeg is included in Neoss 3D libraries for design of matching CAD/CAM abutments in design software from 3shape, Exocad and Dental Wings. The CAD/CAM abutments can be provided with straight or angulated screw channels in Ti, CoCr and ZrO.\*

The following versions and higher of the Neoss Brand Library are compatible with the Esthetic Healing Abutments with ScanPeg:

- 3shape: Neoss Brand Library 0.8
- Exocad: Neoss Brand Library 0.5
- DWOS: Neoss Brand Library 0.4

The libraries are available for download, together with the installation and ordering guidelines and order forms, on [www.neoss.com/cad-libraries](http://www.neoss.com/cad-libraries).

*\*Contact your local representative for availability on your market. Certain design software have limitations in combining intraoral scan with ScanPeg and angulated screw channels.*

In addition, the ScanPeg is compatible with the Cerec Omnicam scanner from Sirona Dentsply and the inLab designs SW 4.x software. The compatibility is based on referring to the Sirona Dentsply ScanPost and Scan Body during the model making and design for the Neoss TiBase. It is also possible to export and use the design file created in inLab for production of a Neoss Individual Abutment.

The Esthetic Healing Abutments are part of the Esthetiline range and like the Tissue Formers match the profiles of stock abutments – Preable Abutments, Zirconia Abutments and NeoLinks.

# Esthetiline overview – stock abutments and conventional impression taking

## Product Assortment

Prepable Abutments



Zirconia Abutments



NeoRose® Mono



NeoLink® Mono



## Esthetic Restoration

## Impression Solutions

Esthetic Tissue Formers



## Temporary Solutions



## Soft Tissue Healing


Esthetic Healing Abutments








Ø3.5 – Ø6.0

## Treatment Options



Screw Retained



Cement Retained/Chairside



## Indexing



# Esthetiline Shapes

Stock abutments

Prepable Abutments




Zirconia Abutments




Digital Abutments

NeoBase Abutments

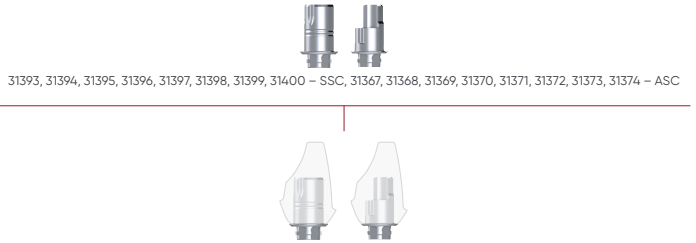

Esthetic Tissue Formers

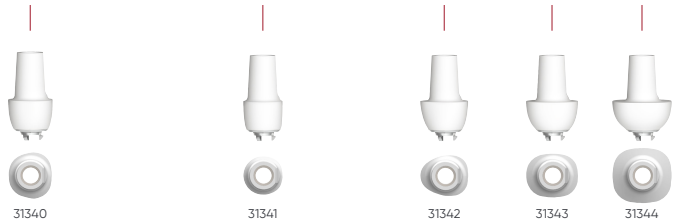

Digital library shapes



Esthetic Healing Abutments



Wide Incisor

Narrow Incisor

Canine

Pre-molar

Molar

# Final restoration – stock abutments

## Prepable Titanium Abutment

The shape of Prepable Titanium abutments match the profile of the Tissue Formers making it possible to accurately define soft tissue contours without the need for complex impression procedures. The abutments may be modified by marginal adaptation and angulation. For more information about Prepable Titanium Abutments please refer to section "3.8 Titanium Prepable Abutments".

## Zirconia Abutment

Zirconia abutments are supplied in two parts; the Zirconia coping, with a profile matching the provisional Tissue Formers thus giving an optimal aesthetic solution, and a pre-blasted Titanium NeoLink® Mono. The Zirconia coping is designed to be cemented onto the NeoLink®. This may be carried out at the chair-side or in laboratory using resin bonded cement. Careful adjustment of the ceramic coping may be made prior to cementation and placement. For more information about use of the Zirconia abutment please refer to section "3.9 Zirconia Abutment".

## NeoLink® Mono and NeoLink® Plastic Copings

*Note: Plastic copings can be used with a NeoLink® as try-in abutments to facilitate abutment selection. Plastic copings are for single use.*

There is an index between the NeoLink® and the coping in order to achieve a specific orientation in relation to the implant's rotational position.

For more information about custom abutments and copings and CAD/CAM solutions please refer to section "3.4 NeoLink® – Gold/Titanium".


## 4.1.4 Neo and iGO screw overview



Healing abutments, impression copings, provisional abutments and permanent abutments are all attached by using specific Neo screws and Neo screwdrivers as described in the subsequent sections. The only exception to use the Neo screwdriver is for angulated screw channels (ASC) where iGO screws are required together with the iGO screwdriver.

## Screw and screwdriver compatibility

### Neo screws and Neo screwdriver

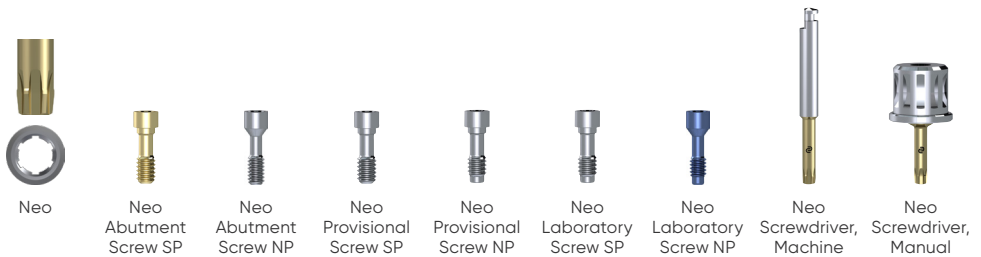





Note: iGO screws and Neo screws are visually differentiated by conically shaped and partially coated screw head.

Note: Abutment and laboratory screws are visually differentiated by coating and by number of threads.

Note: Identification of Neo Abutment screw vs Provisional Screw and Laboratory screw.



## 4.2 Impression Techniques

Neoss offers a range of solutions for accurate and fast impression taking on both implant and abutment level using intraoral scanning or conventional impression techniques.

### 4.2.1 Digital impressions

Neoss Scan Bodies are available for all Neoss implants and Neoss Access and Multi-Unit abutments. In addition, Neoss offers the ScanPeg which is a scan body momentarily fitted in the screw access hole of the Neoss Esthetic Healing Abutment. The combination of these two components is used to take a digital impression without removing the healing abutment from the implant.

Neoss Scan Body and ScanPeg are compatible with most available scanners and planning and design softwares. Neoss CAD Libraries can be downloaded from [www.neoss.com](http://www.neoss.com).

#### Digital impression with Neoss Scan Body




The Scan Body is secured to the implant/abutment using a specific integrated screw. The Scan Body is made of titanium which is visible on x-ray if the user wants to confirm proper seating.



#### Clinical Procedure – Scan Body


1. Use the Scan Body as supplied.

Note: Neoss Scan Body SP and NP are 'self-seating'. This means that the screw will not engage the implant if the scan body is not correctly seated. However, a radiograph is recommended if there is any uncertainty or risk of soft tissue entrapment.



2. Expose the head of the implant or abutment – e.g. remove the cover screw or healing/provisional abutment and ensure that the top of the implant is clear of any soft or hard tissue.
3. Place desired scan body (SP, NP, Access, Multi-Unit) onto the implant or abutment and tighten the screw – hand tightening is sufficient, use the Neo screwdriver and manual handle.
4. Conduct the scan according to the scanner manufacturer's instructions
5. Using the Neo screwdriver ensure that the screw has been completely undone/disengaged from the implant or abutment and remove the scan body.
6. Remount the cover screw or healing/provisional abutment to cover the head of the implant or abutment.

### Clinical Procedure – ScanKey



When using multiple Scan Bodies, ScanKeys can be used to bridge the edentulous gap between Scan Bodies to aid in the scanning process. The ScanKey provides a scannable bridge between the Scan Bodies.

Follow the workflow above with the following additional steps:

1. Download the STL-file and print the Scan Key Kit using any of the validated\* resin materials.

\* ScanKeys have been validated for the following materials:  
Sprinray Study Model White 2.

2. If a shorter ScanKey is required, cut or break off sections from the ScanKey.



3. Clip on the ScanKey in the matching groove on the Scan Body before scanning.



4. The ScanKeys can be used to construct a transfer jig for a verification model. Connect the ScanKeys and Scan Bodies using a non-resilient light curing material and transfer to the verification model.

### Digital impression with Esthetic Healing Abutment and ScanPeg


The Esthetic Healing Abutments have a specific non-exchangeable screw and are designed to enable the ScanPeg to be fitted in the healing abutment with a press-fit.

The ScanPeg is designed to fit the screw access hole of the Esthetic Healing Abutments. The combination of these two components is used to take a digital impression without removing the healing abutment from the implant.

## Procedure

### Healing abutment placing and screw access hole protection:

The abutment profile of the gingival margin is fixed in relation to the non-rotational feature on all Esthetiline abutments and thus related to the position of the implant – indexing. The Esthetiline solution is best applied by ensuring one groove in the implant to be oriented in the buccal direction during implant installation. This will require the least adjustment. Indexing throughout the treatment is possible utilizing the indexing features as shown.



The groove inside the Esthetic Healing Abutment is oriented buccally when placed in the implant. The Esthetic Healing Abutment is tightened to a maximum of 10 Ncm.

or

*Note: The height of the Esthetic Healing Abutments shall not be adjusted since the scanning accuracy can be impaired. However, minor adjustments of the gingival profile may be carried out by grinding with a bur as the material is PEEK.*

In order to protect the screw channel and thereby the scanning accuracy, fill the cavity with a PTFE tape alternatively silicon impression paste at placement.

### Cleaning the screw access hole prior to ScanPeg seating:

Clean the screw access hole thoroughly without using sharp instruments that can damage the inside and the ScanPeg seating.


### ScanPeg seating and scanning:

#### Correct seating

When correctly placed, the ScanPeg will rest on the shelf inside the screw channel and the upper edge of the horizontal groove will be flush with the healing abutment.

The ScanPeg is incorrectly seated if the horizontal groove is clearly visible.

*Note: The groove cannot be used as a as an indicator if the abutment height has been reduced.*

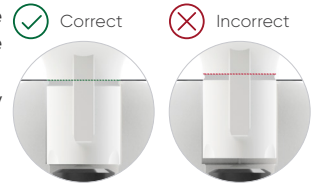

#### Step-by-step

1. Center the ScanPeg in the screw access hole of the Esthetic Healing Abutment.
2. Align the lug on the ScanPeg with the groove inside the Esthetic Healing Abutment.
3. Push in until properly seated.
4. Scan according to the manufacturer's instruction.
5. Pull out ScanPeg and dispose of it.

*Note: Avoid repetitive placements as it can affect the retention.*




## Digital Analogs - Procedure

1. Print a working model with the compatible analog interfaces and the placement tool using the Neoss CAD Library.



2. Place the Digital Analog in the working model. Align the groove in the Analog with the groove in the model. The Analog has a rotational lock and fits in one direction only.



3. Place the placement tool on top of the Digital Analog and press firmly until the Digital Analog clicks into place. The Digital Analog is now securely fixated in the working model.



4. The optional fixation screw can be mounted in the Digital Analog from underneath in cases where an extra firm position is required (e.g. bridge work). Use the Neoss screwdriver to fasten the screw. The torque applied to the fixation screw should be "finger tight" and should never exceed 5 Ncm.



## 4.2.2 Conventional impressions

Implant level impressions may be used to accurately record implant positions easily using open or closed tray techniques for the Neoss System. Exceptions are the Express and Access Abutment which have their own specific copings. Impressions of Titanium Preable Abutments can be taken using conventional crown and bridge method.

The purpose of an implant level impression is to accurately transfer to a laboratory model the position of the implant in relation to natural teeth or other implants as well as the soft tissue contours.

An Implant Level impression may be made at different stages during treatment and is dependant on operator preferences:

- At time of initial surgery – for one stage techniques, or to enable the delivery of a provisional crown at second stage surgery
- At second stage surgery
- Following soft tissue healing after a second stage surgical procedure

The Neoss System offers one universal Implant Level Impression Coping for both 'Open' and 'Closed' Tray impression techniques as detailed below and one Impression Coping for 'Open Tray' impression only.

The universal impression coping is available in three different lengths – 8 mm, 11 mm and 18 mm.

The universal Impression Coping utilizes separate items depending on impression technique and is packaged with the implant replica.

Impression coping – which engages the implant has both horizontal and vertical grooves for definite retention in the impression material.

Screw – which secures the impression coping to the implant during impression taking (use Neo screwdriver in conjunction with manual handle).

Plastic extension tube – which may be trimmed to length and enables easy access to the head of the screw when using the 'Open Tray' technique.

*Note: The impression copings are not interchangeable for reasons of accuracy. Hence use the same impression coping in the same impression cavity.*

Red Plastic Cap – which is used for closed tray impressions only.

Impression Coping Open Tray.



# Neoss Implant Level Impression Techniques

## Open Tray

In an open tray technique the impression coping is 'picked up' in the impression material. Only three of the four components of the universal Impression Coping Assembly are used, the Red and White Plastic Caps are NOT used.



### Clinical Procedure – Open Tray

1. Use the universal Impression Coping as supplied.

*Note: The Neoss Impression coping is 'self-seating'. This means that the screw will not engage the implant if the coping is not correctly seated. However a radiograph is recommended if there is any uncertainty or risk of soft tissue entrapment.*



2. Expose the head of the implant – e.g. remove the cover screw or healing/provisional abutment and ensure that the top of the implant is clear of any soft or hard tissue.
3. Place desired length impression coping (8, 11 or 18 mm) (11 mm for Ø3.25 mm implant) Implant Level impression coping onto the implant and tighten the screw – hand tightening is sufficient, use the Neo screwdriver and manual handle.
4. Try-in the modified impression tray (a window has been previously cut in the area of the implant) and ensure that the tray is clear of the impression coping and the plastic tube extends beyond the impression tray. The plastic tube may be reduced or removed prior to taking the impression. Place some wax over the window.
5. Using a medium to heavy body impression material, inject around the impression coping and fill the impression tray.
6. Seat the impression tray into the patient and ensure the plastic tube/s is clearly visible.
7. After the impression material has set, grasp the plastic sleeve with tweezers and remove.
8. Using the Neo screwdriver ensure that the screw has been completely undone/disengaged from the coping and remove the impression.

*Note: Upon removal of the impression the implants are covered by replacing the cover screw or healing/provisional abutment.*

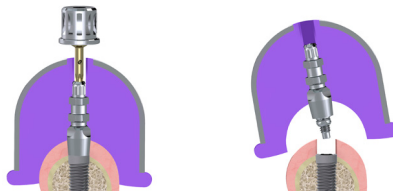

- Using the Neo screwdriver attach the implant replica to the impression coping. Whilst supporting the screw with the screwdriver, ensure correct seating and hand tighten – DO NOT OVER TIGHTEN (10 Ncm maximum).

*Note: The Impression Coping Open Tray utilizes same procedure as above.*

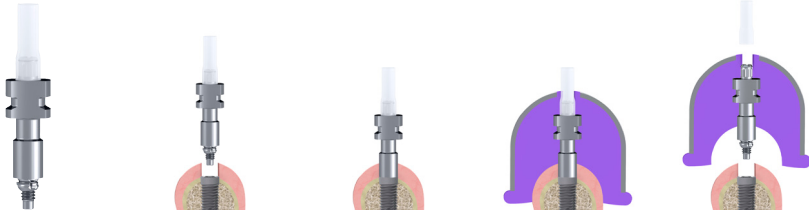

## Neoss Implant Level Impression Techniques

### Closed Tray

In a closed tray technique the impression coping remains in the patient's mouth when the impression is removed. Once the impression coping has been removed and the replica attached it is then re-seated into the impression. The Red Plastic Cap is utilized over the impression coping once it has been correctly seated into the patient's mouth. The plastic extension tube is NOT used.

*Note: This technique may be contraindicated in cases where implant angulation is severe.*



### Clinical Procedure – Closed Tray



- Use the impression coping as supplied – however remove the plastic extension tube.  
*Note: The Neoss impression coping is 'self-seating'. This means that the screw will not engage the implant if the coping is not correctly seated. However a radiograph is recommended if there is any uncertainty or risk of soft tissue entrapment.*
- Expose the implant – e.g. remove the cover screw or healing/provisional abutment and ensure that the top of the implant is clear of any soft or hard tissue.
- Place the desired length impression coping (8, 11 or 18 mm) (11 mm for Ø3.25 mm implant) Implant Level impression coping onto the implant and tighten the screw with the Neo screwdriver and manual handle.

Position the Red Plastic Cap on the impression coping and firmly push until seated.

*Note: The upper part of the Impression Coping has a direction indicator located between the two flat surfaces that aligns with one of the engaging lugs for optimal orientation. The direction indicator is ideally positioned facially for proper seating of the red Impression Coping Cap.*

*Note: Align the flat side of the red Impression Coping Cap with the direction indicator on the Impression Coping to allow for proper orientation of the Impression Coping Cap during seating.*





4. Using a medium to heavy body impression material, inject around the impression coping and fill the impression tray.
5. Seat the impression tray into the patient.
6. When the impression material has set, remove the impression (the Red Plastic Impression Cap is 'picked up' in the impression).
7. Using the Neo screwdriver unscrew and remove the Implant Level impression coping from the patient.
8. The implant replica (supplied with the impression coping) is now screwed into the impression coping.
9. Reposition the impression coping with replica attached back into the corresponding location in the Red Plastic Cap in the impression (use the two flat sides of the impression coping for alignment into the Red Plastic Cap).  
The impression coping needs to be properly oriented in the Red Plastic Cap, meaning that the coping will slide without resistance almost completely down into the cap before a final push seats the coping.

## 4.3 NeoBase® and TiBase Abutments – Digital

### 4.3.1 NeoBase® Abutments




The NeoBase® abutment provides metal support for ceramic restorations whereby the abutment is cemented into the restoration preferably before clinical placement. They are available in Mono and Multi versions for all Neoss implants as well as for both straight and angled screw channels. The NeoBases are a key component of the In-Lab workflow for customized abutments and bridges for ceramic milling of predominately zirconia material.

#### NeoBase® Abutments

##### NeoBase® Abutment SSC

NeoBase® abutment SSC for Straight Screw Channels is delivered with the Neo abutment and Neo laboratory screws.

##### Components and materials

Description	Material	Implant Platform	Screw	Tightening torque	
NeoBase® Mono SSC G0.3 mm – H3.6 mm	Titanium grade 5	SP (Ø3.5–6.5 mm)	 Neo	32 Ncm	
NeoBase® Mono SSC G1.5 mm – H3.6 mm					
NeoBase® Mono SSC G0.3 mm – H5.6 mm					
NeoBase® Mono SSC G1.5 mm – H5.6 mm					
NeoBase® Multi SSC G0.3 mm – H3.6 mm					
NeoBase® Mono SSC G0.3 mm – H3.6 mm, NP		NP (Ø3.25 mm)	 Neo	32 Ncm	
NeoBase® Mono SSC G0.3 mm – H5.6 mm, NP					
NeoBase® Mono SSC G0.3 mm – H5.6 mm, NP					
NeoBase® Multi SSC G0.3 mm – H3.6 mm, NP					



All components might not be available on all markets.




## NeoBase® Abutment ASC

NeoBase® abutment ASC for Angulated Screw Channels ASC is delivered with the iGO abutment and iGO laboratory screws. NeoBase® ASC abutments offer the option to angulate the screw channel up to 25°.

### Components and materials

Description	Material	Implant Platform	Screw	Tightening torque
NeoBase® Mono ASC G0.3 mm – H3.6 mm	Titanium grade 5	SP (Ø3.5–6.5 mm)	 iGO	32 Ncm
NeoBase® Mono ASC G1.5 mm – H3.6 mm				
NeoBase® Mono ASC G0.3 mm – H5.6 mm				
NeoBase® Mono ASC G1.5 mm – H5.6 mm				
NeoBase® Multi ASC G0.3 mm – H3.6 mm				
NeoBase® Mono ASC G0.3 mm – H3.6 mm, NP	Titanium grade 5	NP (Ø3.25 mm)	 iGO	20 Ncm
NeoBase® Mono ASC G0.3 mm – H5.6 mm, NP				
NeoBase® Multi ASC G0.3 mm – H3.6 mm, NP				



All components might not be available on all markets.

## Clinical Procedure Visit 1

The healing abutment is removed in order to expose the implant.

A digital or conventional impression is recorded and sent to the laboratory where a physical or digital master model with implant replica is created.

## Clinical Procedure Visit 2 – Fastening a Custom Made Construction

1. The custom abutment/framework is screwed into the implant using the appropriate abutment screw (Neo for NeoBase SSC and iGO for NeoBase ASC).
2. Once the fit has been verified it is tightened to the recommended torque.
3. If a crown was constructed as a separate unit it is then cemented onto the abutment in the desired manner.

*Note: When cementing a crown onto an abutment the screw access hole should be blocked out with an appropriate material (e.g. gutta-percha) prior to cementation of the crown. When screw retaining a crown direct to the implant the screw access hole should be filled with a small amount of removable material then overfilled with a permanent material (e.g. composite resin).*

4. The occlusion and retention are checked and verified.

## 4.3.2 Neoss TiBase Abutments and ScanPost

The TiBase abutments provides metal support for ceramic restorations whereby the abutment is cemented into the restoration preferably before clinical placement. The Neoss TiBase abutments and ScanPost are designed to be compatible with the TiBase solution and the inLab designs SW 4.x software within Sirona Dental CAD/CAM-System provided by Sirona GmbH.

### Neoss® TiBase Abutments and ScanPost

#### Neoss TiBase Abutment

TiBases are compatible with the inCoris ZI meso blocks from Sirona Dental System. All digitally designed copings and/or crowns for use with the TiBases are to be designed and milled using the Sirona Dental CAD/CAM-System.

The TiBase SP are available in two sizes, N and W, to account for different emergence profiles, while the TiBase NP is available in one dimension. TiBases are delivered with a Neo abutment screw and a laboratory screw. All articles are delivered non-sterile and intended for single use only. TiBases are used in combination with taking digital impressions to record implant position in relation to topographical characteristics of neighboring teeth and soft tissue.

Individually manufactured final or provisional restorations can be cemented onto the TiBase, before being fastened to the Neoss implants with the abutment screw in the mouth. Scanbodies provided by Sirona Dental Systems GmbH are compatible with the TiBase for design in CEREC SW/inLab SW software.

### Neoss TiBase ScanPost

The ScanPost is used only for digital acquisition of the implant position in relation to the remaining teeth and soft tissue using a scanbody mounted on the ScanPost. ScanPosts can be used intraorally and extra-orally.

There are two ScanPosts, SP and NP. The ScanPost and fixing screw are intended to be sterilized following the guidelines in 14077.

*Note: The ScanPost must not be used for the final implant treatment.*

Digital scanning of the implant position with ScanPost is possible only in connection with one of three software products, i.e. CEREC SW 4.2, CEREC Connect SW 4.2 or inLab SW 4.2 (or higher).

### Components and materials

Art. No.	Description	Material	Scan body	Implant Diameter	Compatible with grinding blocks
31329	Neoss TiBase N (NB B 3.4 L)	Titanium grade 5	L	Ø3.5–6.0 mm	Sirona: inCoris ZI meso, size L
31330	Neoss TiBase W (NB B 4.1 L)	Titanium grade 5	L	Ø3.5–6.0 mm	Ivoclar Vivadent: IPS e.max CAD, size L
31331	Neoss ScanPost L (TiBase)	Stainless steel	L	Ø3.5–6.0 mm	–
31345	Neoss TiBase Ø3.25 (FX 3.4 S)	Titanium grade 5	S	Ø3.25 mm	Sirona: inCoris ZI meso, size S Ivoclar Vivadent: IPS e.max CAD, size S
31346	Neoss ScanPost S (Ø3.25 TiBase)	Stainless steel	S	Ø3.25 mm	–

*All components might not be available on all markets.*



### Clinical Procedure Visit 1

The healing abutment is removed in order to expose the implant.

A conventional impression is recorded and sent to the laboratory where a master model with implant replica is created, or an intraoral digital impression using the TiBase ScanPost as below can be taken.

### Clinical Procedure Visit 2 – Fastening a Custom Made Construction

1. The custom abutment is screwed into the implant using the appropriate Neo abutment screw.
2. Once the fit has been verified it is tightened to the recommended torque.
3. If a crown was constructed as a separate unit it is then cemented onto the abutment in the desired manner.

*Note: When cementing a crown onto an abutment the screw access hole should be blocked out with an appropriate material (e.g. gutta-percha) prior to cementation of the crown. When screw retaining a crown direct to the implant the screw access hole should be filled with a small amount of removable material then overfilled with a permanent material (e.g. composite resin).*

4. The occlusion and retention are checked and verified.



Correct mounting of scanbody on ScanPost or TiBase

## 4.4 NeoLink® – Gold/Titanium

### Introduction

The Neoss Implant System abutments have been designed to facilitate the fabrication of custom designed screw retained gold, titanium and ceramic abutments or frameworks having a precision machined fit which are utilized in the production of cement or screw retained implant prosthesis.

Neoss abutments offer high accuracy prosthetic solution.

Abutments and frameworks may be produced in zirconia or other options such as gold, titanium or cobalt chrome, or they may be CAD/CAM produced while maintaining the accuracy and tolerances obtained from machined components. This is possible due to the NeoLink®, which is a precision machined component made of gold, c.p. titanium or cobalt chrome, providing the interface between implant and abutment framework.

Once the accuracy of the Neoss replica has been checked on the master model, the choice is made to create a crown (NeoLink® Mono) or bridge (NeoLink® Multi) in gold, titanium or cobalt chrome. A custom abutment or framework is produced by combining the most appropriate design of plastic anatomical coping with the desired NeoLink®.

There are a number of options:

1. CAD/CAM abutments/frameworks cemented or bonded to the NeoLink/s® titanium.

*Note: Bonding of CAD/CAM designed copings or frameworks may be done 'prior to' or 'after' application of the porcelain/restorative material. This depends on the materials and techniques utilized.*

2. Invest and cast directly onto the gold NeoLink® with a suitable alloy.


3. Remove the NeoLink® from the waxed coping/framework and cast the anatomical coping/framework (in a desired alloy) without the NeoLink®. After proper finishing of the cast coping/framework bond to the NeoLink/s® or laser weld (cobalt chrome).

*Note: The margin on the titanium abutments is too thin to be used in conjunction with welding a cast coping/framework to the NeoLink®.*

Three types of restorations can be produced; a restoration cemented on to custom abutments, a framework retained directly on the head of the implant by abutment screws, or an angulated screw retained solution using Access abutment.

Because the cast abutment or framework can be bonded to the precision machined NeoLink® a true passive fit can be achieved. Inaccuracies caused in casting or porcelain firing can therefore be eliminated. Generally connection by cementation or bonding is carried out in the laboratory after the application of the restorative material. All metals, alloys and ceramics can be bonded to NeoLinks®, including cobalt chromium for example.

*Note: It is possible to cast gold abutments or frameworks in the same manner as titanium in that it may be cast separate to the NeoLink®. Therefore the possibility exists to have a prosthesis completed in a gold alloy with conventional PFM techniques, then bonded or cemented to a titanium NeoLink® – this results in a titanium precision machined interface between the implant and the abutment.*



Gold and Ti NeoLink® Mono



Gold and Ti NeoLink® Multi

Note: Identification of Neo abutment screw vs Laboratory screw and Provisional Screw.



## 4.4.1 Single Unit Construction

Individual crowns may be constructed in one of two ways. The selected option will depend on clinical preferences, angulation of the implant and aesthetic demands:

- As an integral screw retained crown/abutment attached directly to the implant (use NeoLink® Mono).
- As a two part restoration with a custom screw retained abutment and a cement or lingually screw retained crown (use NeoLink® Mono).

Note: A NeoLink® is supplied with two straight copings, with and without margin.

Note: Minimum abutment height from the implant interface is 4 mm.

### Clinical Procedure Visit 1

1. An implant level impression is recorded and sent to the laboratory.

### Clinical Procedure Visit 2

1. The custom abutment is screwed into the implant using the appropriate abutment screw.
2. Once the fit has been verified it is tightened to the manufacturer's recommended torque. For the Neo abutment screw the recommended torque is 32 Ncm.
3. If the crown was constructed as a separate unit it is then cemented onto the abutment in the desired manner.

Note: When cementing or lingually screw retaining a crown onto an abutment the screw access hole should be blocked out with an appropriate material (e.g. gutta-percha) prior to cementation of the crown. When screw retaining a crown direct to the implant the screw access hole should be filled with a small amount of removable material then overfilled with a permanent material (e.g. composite resin).

4. The occlusion and retention are checked and verified.

## 4.4.2 Multiple Unit Construction

Multiple Unit implant supported bridges may be constructed in one of three ways. The selected option will depend on clinical preferences, angulation of the implant/s and aesthetic demands:

- As an integral screw retained one piece bridge attached directly to the implants (use NeoLink® Multi).
- As a cement retained or lingually screw retained bridge over 'individual' custom abutments which have been screwed direct to the implants (use NeoLink® Mono).
- As a screw retained bridge attached to implants via angulated or straight Access abutments, described in section 3.12.

Note: A NeoLink® is supplied with two straight copings, with and without margin.

Note: Minimum abutment height from the implant interface is 4 mm.

### Clinical Procedure Visit 1

1. An implant level impression is recorded and sent to the laboratory.

## Clinical Procedure Visit 2

1. The abutments or framework are screwed into the patient's mouth using the abutment screws.
2. Once the fit has been verified it is tightened to the manufacturer's recommended torque. For the Neo abutment screw the recommended torque is 32 Ncm.
3. If the bridge is constructed as a separate unit it is then cemented or lingually screwed onto the abutments/framework in the desired manner.

*Note: When cementing or lingually screw retaining a bridge onto abutments the screw access holes should be blocked out with an appropriate material (e.g. gutta-percha) prior to cementation of the bridge. When screw retaining a bridge direct to the implants the screw access holes should be filled with a small amount of removable material then overfilled with a permanent material (e.g. composite resin).*

4. The occlusion and retention are checked and verified.

### 4.4.3 Double Scan – Milled Constructions

As part of Neoss Individual Prosthetics, Neoss offers milled abutments, frameworks including bars in different materials on selected markets, for further information contact your local Neoss representative.

#### Laboratory Procedure – Double Scan

For CAD/CAM systems providing double scan features we recommend the following procedure to ensure that the screw access hole is correctly read and scanned by the scanner, and to ensure that it is pre-prepared into the abutment/frameworks:

1. After final waxing/preparation of the abutment/framework on the model, insert an extension from the NeoLink® to the outer surface of the screw access hole in the pre-formed plastic coping. Round plastic tube/rod of 2.5 mm diameter may be used (alternatively use the impression coping screw).
2. This extension tube is trimmed 'level to' (or minimally above) the screw access hole in the preformed plastic coping.
3. Spray with scanning powder/paint if recommended by the CAD/CAM provider.
4. Remove waxed abutment from the NeoLink® – being careful to leave the extension tube in correct position.
5. Spray exposed extension tube and NeoLink® with scanning powder/paint if recommended.
6. Scan the NeoLink® with the extension tube as the FIRST scan in the scanner.
7. Place the waxed abutment onto the NeoLink® and do the SECOND scan – following the specific CAD/CAM manufacturer's manual for double scanning techniques. This process will create a thin shell of material (ceramic, metal) over the screw access hole, which is easily removed prior to sintering, or after sintering by careful grinding for a ceramic restoration.
8. When a milled and sintered coping has been created it is then cemented on the NeoLink® by:
  - A. Sandblasting the NeoLink® with aluminium oxide of 50–100 microns – do not sandblast fitting surface of NeoLink®, use replica to protect the fitting surface.
  - B. Apply a resin bonded cement to the NeoLink® according to manufacturer's instructions.
  - C. Bonding the milled coping onto the NeoLink® with a preferred cement – according to the cement manufacturer's recommendations. An opaque cement is optimal. Please refer to the cement recommended by the CAD/CAM provider.

#### Clinical Procedure – Fastening a Custom Made Construction

1. The custom abutment/framework is screwed into the implant using the appropriate abutment screw.
2. Once the fit has been verified it is tightened to the manufacturer's recommended torque. For the Neo abutment screw the recommended torque is 32 Ncm.

3. If a crown was constructed as a separate unit it is then cemented onto the abutment in the desired manner.

*Note: When cementing or lingually screw retaining a crown onto an abutment the screw access hole should be blocked out with an appropriate material (e.g. gutta-percha) prior to cementation of the crown. When screw retaining a crown direct to the implant the screw access hole should be filled with a small amount of removable material then overfilled with a permanent material (e.g. composite resin).*

4. The occlusion and retention are checked and verified.

## 4.5 Multi-Unit Abutment



### Indications

- Multiple unit screw-retained restorations with straight or angulated screw access
- Fully or partially edentulous cases
- Retrievable restorations



### Material

- Abutment – Titanium
- Screw – Titanium



### Assortment

- Straight: 1, 2, 3 and 4 mm
- Angulated: 10° 2, 3 and 4 mm, 17° 2.5, 3.5 and 4.5 mm and 30° 3, 4 and 5 mm



Multi-Unit Abutments,  
Straight and Angulated

## General

The Multi-Unit Abutment design has wide-ranging applications for the Neoss system by enabling screw-retained straight and angulated restorations to be produced. Angulation may be as little as 10° with 4.5 mm of interocclusal clearance.

The Multi-Unit Abutment provides an axial straight or angulated extension to the implant. This facilitates working to, and restoration on, abutment level rather than directly on the implant. The angulated 10°, 20° and 30° Multi-Unit abutments optimize the screw access channel for implants with unfavourable angulations.

Restorations based on NeoBases or burnout abutments can be made in ceramic, cobalt chrome or gold.


An abutment level impression is the procedure of choice to transfer the abutment location to the model.

Multi-Unit Abutments are delivered sterile.

# Multi-Unit Abutment Placement

## Clinical Procedure


1. Select appropriate Multi-Unit Abutment using Neoss Angulation Gauge SP.

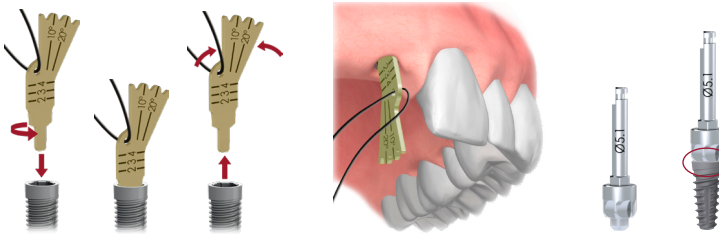

2. It is recommended that a Bone Profiler be used to remove any bone above the restorative platform of the Neoss ProActive implant to ensure correct seating of the Multi-Unit abutment.
3. *Multi-Unit Abutment, Angulated:* The selected angulated abutment engaged with the Neo screwdriver is positioned in the implant and oriented in the correct position (six possible positions) using the pre-mounted abutment holder. For correct orientation it is recommended the Neoss ProActive implant is placed so that one of the internal grooves is aligned Meso/Distally. A unique feature of the angled Multi-Unit abutment is that the abutment will 'hold' into the implant and not dislodge whilst the screw is being inserted.  
*Multi-Unit Abutment, Straight:* The appropriate straight abutment is placed on the implant and screwed into position.

4. Final tightening of the abutment screw to 32 Ncm is carried out using the ratchet and Neo screwdriver.
5. The disposable holder is removed from the abutment.


*Note: The Multi-Unit abutments is preferably mounted at implant surgery or at second stage surgery for optimal tissue healing. Placement in already healed tissue might require additional soft tissue surgery for adequate seating of the angulated abutments. A radiograph may be taken to confirm accurate seating of the abutment.*

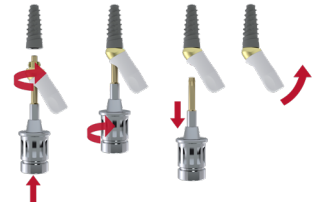

Positioning and tightening of abutment

## Impression Procedure and Provisionalizing

1. Position the Multi-Unit Impression Coping onto the abutment and tighten the coping screw. The impression procedures, open or closed tray, are described in section "3.2 Impression Techniques". The impression is sent to the dental laboratory.
2. Place a Multi-Unit Healing Caps or a Temporary restoration, see sections "1.4 Clinical Treatment" and "3.7.2 Provisional Titanium Abutments". Please note instructions related to the implant level also correspond to Multi-Unit abutment level.

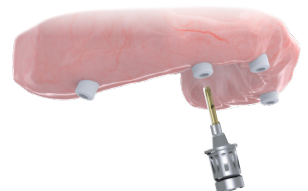

Placement of Healing Abutment



Placement of final restoration

## Final Restoration Placement

1. Remove the Multi-Unit Healing Abutment or the temporary restoration from the abutment.
2. Connect the restoration to the abutment with prosthetic screws. Start with the central screw (if applicable) and tighten the remaining screws alternating between left and right sides.
3. Tighten the prosthetic screws to 20 Ncm using the ratchet and the Neo screwdriver.
4. Block out the screw access channel with gutta-percha. Use a suitable material such as light curing composite to fill in the screw access channel.

## 4.6 Access Abutment



Access Abutments,  
Straight and Angulated

### Indications

- Multiple unit screw-retained restorations with straight or angulated screw access
- Fully or partially edentulous cases
- Retrievable restorations

*Note: The use of angulated Access Abutments for a bridge restoration on two small diameter implants is not recommended for the posterior region. Access Abutments are not available for Ø3.25 mm implants.*

### Material

- Abutment – Titanium
- Screw – Titanium

### Assortment

- Straight: 1.5, 3 and 4 mm (other heights available upon request)
- Angulated: 10° 2.6 and 4.6 mm, 20° 2.6 and 4.6 mm and 30° 2.9 and 4.9 mm

## General

The Access Abutment design has wide-ranging applications for the Neoss system by enabling screw-retained straight and angulated restorations to be produced. Angulation may be as little as 10° with 4.5 mm of interocclusal clearance.

The Access Abutment provides an axial straight or angulated extension to the implant. This facilitates working to, and restoration on, abutment level rather than directly on the implant. The angulated 10°, 20° and 30° Access abutments optimize the screw access channel for implants with unfavourable angulations.

Restorations based on NeoLinks® can be incorporated into gold, ceramic or solid frameworks in titanium, ceramic or cobalt chrome.

Overdenture options are available by utilizing Access Ball and Equator abutments.

An abutment level impression is the procedure of choice to transfer the abutment location to the model.


Access Abutments are delivered sterile.




# Access Abutment Placement

## Clinical Procedure

1. Select appropriate Access Abutment using Neoss Angulation Gauge SP.

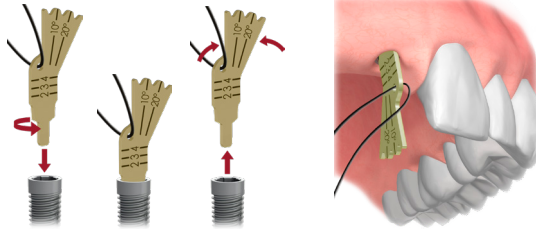

2. *Access Abutment, Angulated:* The appropriate angulated abutment is placed on the implant and oriented in the correct position (six possible positions) using the pre-mounted abutment holder. Keep the pressure on the holder to avoid rotation of the abutment when tightening the screw. The Access Neo abutment screw is then tightened using the Neo screwdriver.  
*Access Abutment, Straight:* The appropriate straight abutment is placed on the implant and screwed into position using the Neo screwdriver.

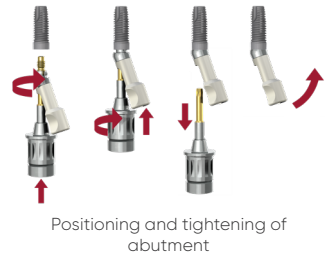


3. Final tightening of the abutment screw to 32 Ncm is carried out using the ratchet and Neo screwdriver.
4. The disposable holder is removed from the abutment.

*Note: The angulated abutment is preferably mounted at implant surgery or at second stage surgery for optimal tissue healing. Placement in already healed tissue might require additional soft tissue surgery for adequate seating of the angulated abutment. A radiograph can be taken to confirm accurate seating of the abutment.*

## Impression Procedure and Provisionalizing

1. Position the Access Impression Coping (lasermarked) onto the abutment and tighten the coping screw. The impression procedures, open or closed tray, are described in section "3.2 Impression Techniques". The impression is sent to the dental laboratory.
2. Place an Access Healing Abutment or a Temporary restoration, see sections "1.4 Clinical Treatment" and "3.7.2 Provisional Titanium Abutments". Please note instructions related to the implant level also correspond to Access abutment level.

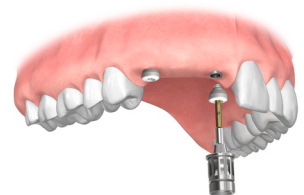

Placement of Healing Abutment



Placement of final restoration

## Final Restoration Placement

1. Remove the Access Healing Abutment or the temporary restoration from the abutment.
2. Connect the restoration to the abutment with prosthetic screws. Start with the central screw (if applicable) and tighten the remaining screws alternating between left and right sides.
3. Tighten the prosthetic screws to 20 Ncm using the ratchet and the Neo screwdriver.
4. Block out the screw access channel with gutta-percha. Use a suitable material such as light curing composite to fill in the screw access channel.

## 4.7 Provisional Abutments



### 4.7.1 Esthetic Tissue Formers

The Esthetic Tissue Former may be used for cement or screw retained single tooth provisional restorations. The abutments may be placed directly into the patient's mouth and prepared intraorally or adjusted by the technician on a laboratory model. If the Esthetiline Solution is utilized, then the optimal result is achieved by choosing the same type of permanent restoration and same position as during healing. The appropriate Esthetic Tissue Former is selected in relation to tooth position for the proposed implant. For improved tissue support, the abutment should be placed so that the margin is supra- or equigingival.

The "chimney" portion of the abutment and the margin height may be adjusted by use of a rotary instrument. In addition, the tissue facing axial contours of the abutment may be modified to achieve the desired shape. If axial modification is done, polishing with silicone points or similar methods is recommended.

*Note: The provisional restoration should be placed out of occlusion.*

*Note: The Esthetic Tissue Former may be adjusted to a minimum diameter of 5.0 mm and to a minimum height of 4.0 mm from the implant platform. The "chimney" portion may be shortened but not narrowed.*


*Note: For provisional bridge restorations Provisional Titanium Abutment Multi is recommended.*



### Screw retained


1. Cut mechanical retention grooves or slots into the Esthetic Tissue Former.
2. Construct a provisional crown in conventional manner. Ensure the screw access channel remains clear. Unscrew and remove the provisional abutment and contour margins/polish etc. as required.

3. Insert the completed provisional crown and tighten to 20 Ncm.

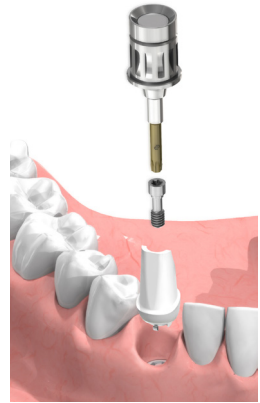


## Cement retained

1. Insert the Esthetic Tissue Former and tighten to 20 Ncm.  
*Note: no additional retention is required*
2. Construct a provisional crown in conventional manner. Ensure the resin does not bond to the Esthetic Tissue Former by for example using a separating medium.
3. It is important to remove and replace the provisional crown at least once prior to final setting of the restorative material to avoid difficulty in removing the crown once the restorative material has set.
4. Contour margins/polish etc. as required.
5. Cement provisional crown onto Esthetic Tissue Former with preferred temporary cement. Care should be taken to ensure that all excess cement is completely removed.  
The provisionals are left in place for desired period, maximum 30 days.



## 4.7.2 Provisional Titanium Abutments

The Provisional Titanium Abutments are designed with a 0.7 mm collar and are available both for single unit (Mono) and multiple unit (Multi) situations. The Mono is available both with and without retention rings (screw retained and cement retained). All Provisional Titanium Abutments come with a plastic coping. The abutments may be prepared intraorally, extra-orally or adjusted by the technician on a laboratory model. Care should be taken when preparing titanium intraorally.



The component may also be used as a waxing sleeve when constructing a crown/framework that will be scanned to produce CAD/CAM prosthesis or copy milled prosthesis.

*Notes: When using the Titanium Provisional Abutment as a waxing sleeve it is recommended to use a self curing resin direct to the abutment.*

*Use the dedicated article Provisional Ti Abutment Mono Cement-retained for cemented cases.*

*Both ends of the plastic coping fit the abutment. One end is straight and the other has a small margin to adapt to the clinical situation. There is an indexing between the plastic coping and the Provisional Abutment (the plane on the Provisional Abutment matches a plane in the plastic coping) in order to achieve a specific orientation in relation to the implant's rotational position.*

For protection and extension of the screw access hole use Laboratory Screw – Long.

The provisional restoration should be placed out of occlusion.

If the plastic coping is utilized, the provisionals can be left in place for desired period maximum 30 days.


## Screw retained

Screw retained provisional crowns/bridges may be produced directly in the patient's mouth (chair-side) or in the dental laboratory.

### Chair-side construction

A provisional crown or bridge may be produced at the chair-side using standard techniques.

In the majority of cases when constructing a screw retained provisional crown/bridge the restorative material is applied direct to the Provisional Abutment, but the plastic coping can be used and bonded as for cement retained solution.



1. For single unit construction use the Provisional Titanium Abutment Mono.  
For multiple unit screw retained direct to implant construction – use Provisional Titanium Abutment Multi.

2. Screw retain the Provisional Titanium Abutment directly to the implant with the appropriate screw – at this time hand tightening is sufficient and cut and adjust by selective grinding as required.

*Note: Adjustments to the abutment are made with high-speed grinding using either a tungsten or diamond bur with irrigation and high volume aspiration.*

*Tip: It is sometimes easier to mark the abutment where it needs adjusting whilst in the mouth, then remove and adjust.*

3. Construct a provisional crown/bridge in the conventional manner. The restorative material is applied direct to the abutment.
4. Unscrew and remove the provisional crown/bridge and contour margins/polish etc. as required.
5. Insert the completed provisional crown/bridge and tighten to 20 Ncm.

### Laboratory construction

#### Clinical step 1

1. An implant level impression is taken and sent to the laboratory.

#### Clinical step 2

1. The provisional crown/bridge is delivered to the patient and hand-tightened to the implant. Final checking of occlusion/contours/color is carried out. Once verified the screw is tightened to 20 Ncm.
2. Block out the screw access channel with gutta-percha. Use a suitable material such as light curing composite to fill in the screw access channel.

## Cement retained

### Chair-side construction

1. For single unit construction use the Provisional Titanium Abutment Mono – Cement retained. For bridge constructions, the engaging section is removed by grinding.

*Note: The Provisional Abutment is designed with an anti-rotational flat side. Additional retention should not be required as it could impair the ability to remove the cemented part.*

### Chair-side/Laboratory construction

2. Construct a provisional crown/bridge in conventional manner utilizing the plastic coping. It is important to remove and replace the provisional crown/bridge at least once prior to final setting of the restorative material to avoid difficulty in removing the crown/bridge once the restorative material has set.
3. Contour margins/polish etc. as required.
4. Ensure that the abutment screw has been tightened to a maximum of 20 Ncm before cementing the temporary crown or bridge with preferred cement (for example, Kerr TempBond® or Kerr TempBond® NE). Care should be taken to ensure that all excess cement is completely removed.

## 4.8 Titanium Preparable Abutments

Preparable abutments may be placed directly into the patient's mouth and prepared intraorally or adjusted by the technician on a laboratory model. Care should be taken when preparing titanium intraorally.



The Neoss System offers Titanium Preparable Abutments in various shapes ranging from incisors to molar, angulations (straight 0° and 15°) and heights (1 mm, 1.5 mm and 3 mm) (1 mm only for Ø3.25 mm implant).

Neoss Implant Abutment Connection – NeoLoc® enables alternative emergence profiles to fulfil specific clinical needs related to emergence profiles such as limited spaces or wide constructions. See section "3.8.1 Titanium Preparable Abutment – Alternative Emergence Profiles", for details.

If the shape/contours of the desired abutment/s are not achievable with either of the Titanium Preparable Abutments then it is recommended to custom-design and cast the abutment in the laboratory utilizing a Gold NeoLink® Mono or Titanium NeoLink® Mono, please refer to sections "3.4.1 Single Unit Construction" and "3.4.2 Multiple Unit Construction" of this Handbook, or use blanks for customized preparable abutment by the laboratory.

*Note: The Preparable Abutments may be adjusted to a minimum diameter of 4.0 mm (minimum 3.5 mm on Preparable Abutments NP) and to a minimum height of 1.0 mm from the implant platform. The "chimney" portion may be shortened to a minimum height of 4.0 mm. Ensure the minimum thickness is 0.4 mm.*

*The blanks may be adjusted to a minimum diameter of 4.0 mm and a maximum height of 8.0 mm when maximum angulation of "chimney" portion is 20°, or maximum height of 4.0 mm when maximum angulation of "chimney" portion is 30°.*



# Titanium Prepable Abutments

## – Preparation On Laboratory Model

### Clinical Procedure Visit 1

1. An implant level impression is recorded and sent to the laboratory.

### Clinical Procedure Visit 2

1. The abutment/s is screwed into the patient's mouth using the Neo abutment screw and Neo screwdriver in conjunction with the manual handle.
2. Once the fit has been verified it is tightened to 32 Ncm.
3. The crown or bridge is then seated on the abutments and checked for fit, occlusion, color etc.
4. The prosthesis is permanently cemented using conventional crown and bridge techniques.
5. The occlusion and retention are checked and verified.

# Titanium Prepable Abutments

## – Preparation Intraorally

### Clinical Procedure Visit 1

1. The healing or provisional abutment is removed and the top of the implant is exposed.
2. Appropriate Titanium Prepable Abutment is selected and screw retained to the implant/s or replica using the abutment screw provided. The use of Neo screwdriver and manual handle is required.

*Note: For optimal placement of the abutment and minimal preparation it is recommended the implant has been indexed as described in section 1.2.*

*Hint: If there are any concerns in relation to correct seating of the abutment to the implant than a radiograph should be taken.*

3. Adjustments to the abutment are made with high-speed grinding using either a tungsten or diamond bur with irrigation and high volume aspiration.

*Tip: It is sometimes easier to mark the abutment where it needs adjusting whilst in the mouth, then remove and adjust.*

*Note: Ideally the margins of the abutment should be 1 to 1.5 mm sub-gingival.*

4. Once the ideal contour has been obtained and correct seating of the abutment to the implant has been verified the abutment screw is tightened to 32 Ncm.
5. The screw access hole is then blocked out (e.g. gutta-percha) and a conventional crown and bridge impression is taken. Gingival retraction cord may be used.
6. A temporary prosthesis is made and inserted.
7. The impression is sent to the laboratory for the construction of the prosthesis.

### Clinical Procedure Visit 2


1. The temporary prosthesis is removed and the abutment cleaned of any debris.
2. The prosthesis is inserted and checked for fit, occlusion, color etc.
3. The prosthesis is permanently cemented using conventional crown and bridge techniques.

## 4.8.1 Titanium Preparable Abutment – Alternative Emergence Profiles

Same clinical and laboratory procedures apply as described in section 3.8, except for the details listed below.

### Wide Emergence Abutment

The Wide Emergence abutment utilizes the outer chamfer of the implant flange for seating, enabling a lower and wider emergence profile than the Molar abutment. The Wide Emergence abutment has same indication as standard Preparable abutments.



### Product content and packaging

The Wide Emergence abutment is delivered sterile. It includes abutment, laboratory screw, abutment screw, specific cover screw and specific healing abutment PEEK with screw. The cover screw and the healing abutment with screw are packed so they can be opened separately from abutment and laboratory screw.

### Compatibility

The Wide Emergence abutment is compatible with ProActive Edge, ProActive Tapered & ProActive Straight (lot # equal or higher than 14646) Implant diameters Ø5.0–5.5 mm and ProActive Ø6.0 implants. The Wide Emergence abutment requires a specific healing abutment and specific cover screw for healing. A wide replica (article 31166, Protection Replica – 1 pc) is required for model making and laboratory preparation.

*Note: Use of Wide Emergence abutment should be planned for and parts available for surgical placement for effective treatment.*


### Narrow Emergence Abutments

Narrow Emergence abutments are intended to be used with the Ø3.5 & Ø4.0 mm implants when only limited mesio-distal space is available.

### Product content and packaging

Narrow Emergence abutments are delivered non-sterile and include abutment, laboratory screw and abutment screw.

*Note: If replacement of abutment is required, use same type of abutment or remove tissue from the seating surface if placement of standard platform abutment is required.*



## 4.9 Zirconia Abutment



Zirconia abutments may be used for cement-retained single and multiple unit restorations and screw-retained single unit restorations and can be prepared at the chairside or by the technician on a laboratory model. Zirconia abutments are supplied in two parts; a Zirconia coping, having a range of profiles to match the Tissue Formers, and a pre-blasted Titanium NeoLink® Mono. The Zirconia coping is designed to be cemented onto the NeoLink®.

### Zirconia Abutment – Chairside (preparation and cementation extra-orally)

#### Clinical Procedure Visit 1

1. The healing abutment is removed in order to expose the implant.
2. An appropriate Zirconia abutment is selected.

*Note: Try-in using NeoLink® and plastic copings.*



#### Preparation and cementation extra-orally

3. Screw retain the pre-blasted NeoLink® to a replica/handle with the Neo Laboratory Screw provided.

*Note: Index the flat plane of the NeoLink® in a buccal direction.*

*Note: Try-in the Zirconia coping, if necessary on the implant by screw retaining the pre-blasted NeoLink® to the implant with the Neo Abutment Screw by hand tightening and mark any adjustments needed on the coping.*

4. Modify the coping to achieve the optimal design as described in section "Zirconia coping modification" on page 3:29.
5. After the ideal contour has been obtained, permanently cement the zirconia coping onto the NeoLink® by using conventional techniques.

*Note: Because of the precision fit between the NeoLink® and the Zirconia coping, only a small cement gap is present (20–50 µm). Apply a small amount of cement and ensure that any excess cement is removed. Check that the screw access channel is clear. Apply a resin bonded cement according to manufacturer's instructions to the NeoLink®.*


6. Remove the Zirconia abutment (NeoLink® and Zirconia coping) from the replica/handle.
7. Attach the Zirconia abutment on the implant in the proper orientation and once correct seating of the abutment to the implant has been verified the Neo abutment screw is tightened to 32 Ncm.

*Note: If there are any concerns in relation to correct seating of the abutment on the implant than a radiograph should be taken.*

*Note: Ensure that the Zirconia abutment is clean and dry.*



8. The screw access hole is then blocked out with a suitable material and a conventional crown and bridge impression is taken. Gingival retraction cord may be used.
9. A temporary prosthesis is made and attached to the Zirconia abutment.
10. The impression is sent to the laboratory for the construction of the crown which is sent to the clinician.
11. The crown (or full-ceramic restoration) must be conditioned and cemented according to the manufacturer's instructions.



## Zirconia Abutment – Preparation by Laboratory

### Clinical Procedure Visit 1

1. The healing abutment is removed in order to expose the implant and an implant level impression is taken and sent to the laboratory.

*Note: For Esthetiline, the type of Tissue Former placed at surgery is communicated to lab.*

### Clinical Procedure Visit 2

1. Attach the Zirconia abutment on the implant in the proper orientation. Once correct seating of the abutment to the implant has been verified the Neo abutment screw is tightened to 32 Ncm.

*Note: If there are any concerns in relation to correct seating of the abutment to the implant then a radiograph should be taken.*

*Note: Ensure that Zirconia abutment is clean and dry.*

2. The screw access hole is then blocked out with a suitable material.
3. The crown (or full-ceramic restoration) must be conditioned and cemented/bonded according to the manufacturer's instructions.

## Zirconia coping modification

Adjust the coping outside the mouth by using burs especially manufactured for preparation of ceramics. Use water cooling to avoid micro cracks. Do not overheat the coping.

Work with a low contact pressure.


*Note: The replica can be attached to a handle for better stability during preparation.*

Avoid sharp preparation edges and corners to ensure a good fit between the abutment and all-ceramic crown. Keep corners rounded with a radius of 0.5 mm or more. Ensure that the minimal thickness of the ceramic material is 0.8 mm, minimum diameter 5.0 mm and minimum height of 5.0 mm from the implant platform.

The maximum thickness of the veneering material on top of the coping must not exceed a maximum of 2.0 mm in all directions. It is advised that the prosthetic margin be 0.5–1.0 mm sub gingival – this will allow for easy removal of excess cement.

*Note: Make sure not to damage the titanium implant interface during modification. Any adjustment below the final crown margin should be polished, preferably using a silicon rubber wheel and diamond paste.*

*Note: It is recommended that adjustment of the Zirconia coping is made prior to cementation!*



## 4.10 CoCr Abutment

---

### Procedures

The abutments provide a restorative solution based on welding a CoCr coping or framework to the abutment in the same way as Ti Neolink® is handled. No angle correction is done by the CoCr Abutment, only via Access Abutments in combination with Multi CoCr Abutment for Access. Please consult sections 3.6, 3.6.1, 3.6.2, 3.6.5 and 3.12.3 Laser Welding in this manual for details on Casting, .

*Note: Metal dust from grinding, blasting and polishing is harmful to health and care*

## 4.11 Burnout Abutment

---

The abutments provide a restorative solution based on a burnout coping mounted on a burnout abutment with subsequent direct investing and casting in CoCr or Titanium (only Multi) following guide lines for Gold Neolink®, please consult sections 3.6, 3.6.1, 3.6.2, 3.6.4 in this manual.

## 4.12 Overdenture Solutions

---

Implant supported overdentures are a relatively simple and cost-effective treatment option for many patients. In some cases it is not necessary to construct a new prosthesis as the patient's existing denture may be utilized. Implant supported overdentures may also be used as a provisional prosthesis. There are three ways to retain implant supported overdentures:

- Ball Abutments
- Equator Abutments
- Bar Abutments

The use of ball abutments has traditionally been in the mandible utilizing two implants.

Bar retained overdentures can either be rigid (multiple implants) or resilient (two implants) in design. Resilient designed overdentures are most commonly limited to the mandible and are implant retained and tissue borne. In the maxilla however bar retained overdentures are normally rigid in design and are implant retained and implant borne. Ball abutment and Equator abutment options are available on Access level as well.

### 4.12.1 Ball Abutments

In the mandible two implants are utilized and in the maxilla up to four implants are utilized for a ball retained overdenture.

*Hint: For ball abutments to be a restorative option the implants must be parallel to within 10 degrees of each other.*

When using the Access Ball abutment the instructions below related to the implant level also correspond to Access abutment level.


## Procedure – Ball Abutments Using Patient's Existing Denture

### Clinical Procedure Visit 1

1. The top of the implants are exposed by removing the healing abutments.
2. The appropriate height ball abutments are placed with the ball driver and tightened to 20 Ncm.

*Tip: Ideally the collar of the ball abutment should extend approximately 1 to 1.5 mm above the soft tissue.*

3. The desired Housing is selected. Place the Space Maintainer over the Ball Abutment and seat the Housing. Transfer the position of the Housing to the denture by marking the top of the Housing and placing the denture over the Housing. Prepare a recess in the denture to accommodate the protruding Housing. Try in the denture over the Housing to verify it is fully seated on the ridge without contact onto the Housing. There should be an undercut well into which self curing resin will flow and be retained.

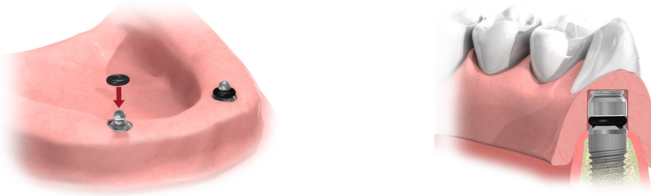

4. The attachment is bonded to the denture using a self curing acrylic or an appropriate attachment cement in the well in the denture. Maintain the denture in a passive condition while the acrylic/resin sets as per the manufacturer's instructions. Once cured, the denture is lifted off the ball abutments together with the embedded Housing. The region of the denture around the attachment is then refined at the chairside or in the laboratory and care is taken to ensure the Housing is not dislodged.

See section "Adjustment and Maintenance" for information about how to insert and change Retention Female in the Titanium Housing.

*Hint: The retentive elements must be placed parallel to each other. A divergence or convergence of up to 10 degrees is acceptable.*

*Note: For completion of the denture in the laboratory, take abutment level impression using existing denture as impression tray. Remove the denture and insert Ball Abutment Replicas in the impression. Pour the master cast, using high quality die stone.*

## Procedure – Ball Abutments Constructing A New Denture

### Clinical Procedure Visit 1

1. The top of the implants are exposed by removing the healing abutments.
2. An implant level impression is taken with Neoss impression copings. The impression should be a full arch impression in a custom made impression tray with either a polyvinyl or polyether impression material.
3. After the material has set the impression is removed from the patient's mouth, the healing abutments are replaced and the provisional prosthesis is returned to the patient. Care should be taken that the provisional appliance does not interfere with the healing abutments. A soft lining material may be utilized in the provisional prosthesis to aid in retention.

*Note: Alternatively, impression can be taken on abutment level.*

### Clinical Procedure Visit 2

1. The corresponding healing abutments are removed and the patient's inter arch/jaw relationship is recorded onto the screw retained bite block/occlusal registration rim.

*Hint: If not all of the healing abutments are removed it will be necessary to relieve the wax registration rim over the healing abutments which have not been utilized in the screw retention of this 'bite block/occlusal registration rim'.*

2. After registration the healing abutments are resealed in the patient's mouth.


### Clinical Procedure Visit 3

1. The waxed prosthesis is evaluated in the patient's mouth, once correct it is returned to the laboratory for processing.

### Clinical Procedure Visit 4

1. The ball abutments are screwed into the implants after removal of the healing abutments and tightened to 20 Ncm using the Neo screwdriver.
2. The denture is returned to the patient and correctly seated.
3. The occlusion and retention are checked and verified.

See section "Adjustment and Maintenance" for information about how to insert and change Retention Female in the Titanium Housing.

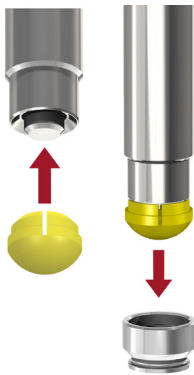

## Adjustment and Maintenance

### Insertion and Removal (Retention Female, Titanium Housing)

Press the Retention Female over the end of the Insertion Tool and press it into the Titanium Housing.

Three retention levels are available: yellow (normal retention) white (reduced retention) and red (increased retention). To remove a Retention Female from the Titanium Housing use a hot pointed instrument.

## 4.12.2 Equator Abutments

### Indications

The Equator Abutment is designed for use with full dentures or partial dentures retained by the Neoss Implants in the maxilla or mandible. The self-locating design allows a patient to easily seat their denture. Restorations with limited vertical space are possible through the 2.1 mm height of the Equator Abutment Housing (the Housing for extended divergence is 2.2 mm). In addition, a 28° divergence (with standard Housing and 50° with Housing for extended divergence) between two implants can be easily accommodated. The divergence between implants can be reduced by using Access abutments.

Either a new denture or the patient's existing denture can be utilized for the construction of an Equator Abutment retained denture. Incorporating the male retentive element into the denture can be made in two ways:

- chairside by the dentist directly into patient's denture in the mouth.
- in the laboratory on a model.

When using the Access Equator abutment the instructions below related to the implant level also correspond to Access abutment level, except for the tightening torque.

*Note: Relining of Equator Abutment retained denture is required to avoid load bearing situation.*

# Contraindications

Not appropriate where a totally rigid connection is required.

Neoss Equator abutments are not recommended for use on a single implant and on implants with a greater divergence than 28° (50° with Housing for extended divergence).

## Caution

Federal (USA) law restricts this device for sale by or on the order of a licensed dentist.

## Sterilization

All components and instruments are supplied NON-STERILE. Implant abutments and metal instruments may be sterilized following standard clinical procedures, prior to use.





## Procedure – New or Existing Denture


### Existing Denture

#### Clinical Procedure

1. The top of the implants are exposed by removing the Healing Abutments.
2. To select the proper Equator Abutment measure the tissue thickness from the apical rim of the implant body to the crest of the gingiva at the highest side of the implant site. Choose the Equator Abutment that exactly equals the tissue measurement, or is the next closest higher size available.
3. It is imperative that all bone and soft tissue is removed from the superior aspect of the implant body to guarantee complete seating of the Equator Abutment. If any doubt, verify complete seating using a radiograph.
4. Hand-tighten the abutment into the implant, using the Neo Screwdriver.
5. The abutment is then torqued to 32 Ncm using the ratchet (20 Ncm for Access level).


Alternatively a torque control device with the Neo Screwdriver can be used.

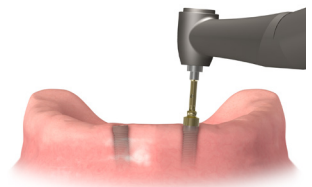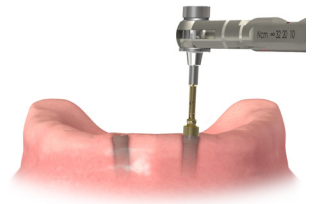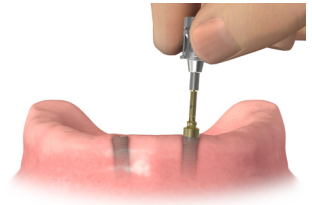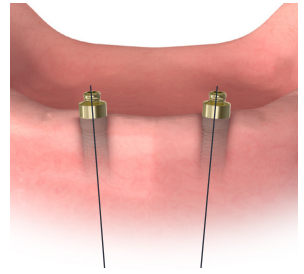



6. Place the Protector Disk over the Equator Abutment (this will prevent acrylic resin from flowing into under-cuts around the housings).

*Note: Make sure the soft tissue is protected from the self curing material.*



7. Place the metal Housing (make sure the Black Processing Cap is inserted into the Housing) onto the Equator Abutment leaving the Protector Disk beneath it.

*Note: The Housing for extended divergence (up to 50°) comes with a specific processing cap.*




8. Prepare a recess in the denture to accommodate the protruding Housing. Try in the denture over the Housing to verify it is fully seated on the ridge without contact onto the Housing.

*Note: Make sure there is NO contact between the denture and the metal Housing.*

9. Use a light cured composite resin or permanent self-curing acrylic to bond the Housing to the denture. Apply a small amount in the recess of the denture and around the metal Housing. Place the denture into position in the mouth and have the patient close into very light contact centric occlusion. Maintain the denture in a passive condition while the acrylic/resin sets as per the manufacturer's instructions.


*Note: It is necessary to block out any remaining undercuts to prevent resin/acrylic from locking the denture onto the abutment.*

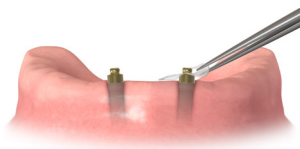

10. After the resin/acrylic has cured remove the denture and discard the Protector Disks. Fill any voids around the Housings and polish.



11. Remove the Black Processing Cap by pushing the tip on the removal side of the Equator Cap Tool firmly aside the internal wall. Push the handle down and the cap will snap out promptly.

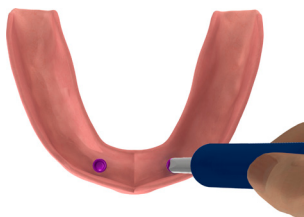

12. Place the final Cap on the end of the insertion side of the Equator Cap Tool and press it firmly into the Housing.

*Note: The attachment retention on the abutment may be reduced by placing the Pink Soft Retention Cap or the Yellow Extra Soft Retention Cap rather than the White Standard Cap.*



*Note: The retention Caps are replaced after normal wear with the Equator Cap Tool as instructed previously.*

13. Upon insertion, check for pressure spots and adjust occlusion.

# New Denture


## Clinical Procedure

1. After inserting the appropriate height Equator Abutment onto the implants in the patient's mouth, place the Equator Impression Copings on the abutments and verify that it is correctly seated.
2. A medium or heavy body impression material is recommended. Syringe the impression material around each of the entire Equator Impression Copings. Load the impression tray or patient's existing denture and seat in the mouth. Allow the impression material to set per the manufacturer's instructions.

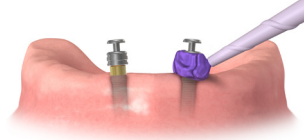


3. Remove the impression from the mouth and verify that the impression material completely adapted around each coping. The Impression Copings should remain inside the impression.

*Note: The Impression Coping comes with the Yellow Extra Soft Retention Cap instead of the Black Processing Cap for optimized compromise between stability and retention.*




4. Snap an Equator Replica (2 supplied in each Impression Coping pack) onto each Impression Coping in the impression.

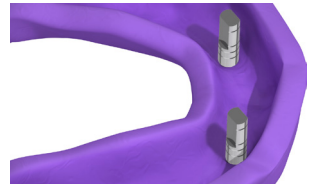

## Choice of Neoss Equator Retention Caps

Patients should be able to insert and remove their Equator retained dentures simply and reliably.

To use the Equator components the divergence for the Equator Abutment must not exceed 14° (or 28° in the case of two abutments) alternatively 25° (or 50° in the case of two abutments) if the Housing for extended divergence is utilized.

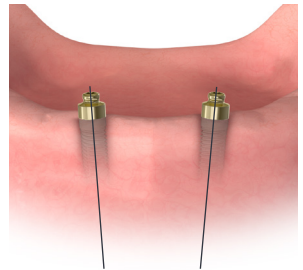

## Multiple Equator Abutments

If several (3 or more) Equator Abutments are used in the same jaw, we recommend using either:

- the Pink Soft Retention Cap with retention of 1.2 kg.

Or:

- the Yellow Extra Soft Retention Cap with retention of 0.6 kg.

# Converging or diverging Equator Abutments

In the cases where implant divergences exceed 28° (in the case of two abutments), we recommend to use Access abutments to reduce the divergence or the Housing for extended divergence (50° in the case of two abutments).

## Patient care

Good oral hygiene is vital to implant success. The Equator Abutment must be thoroughly cleaned daily. The use of a soft nylon bristle or end-tufted toothbrush, and super floss to polish the abutments should be taught.

A non-abrasive gel toothpaste, and an irrigation system is recommended to keep the socket of the Equator Abutment clean.

Patients should maintain a three to four month recall for cleaning and implant evaluation.

The sulcus area around the implant abutment is the primary area of concern.

Use plastic instruments for scaling the abutments. Do not use metal instruments which may create scratches on the abutment surface. Examine patients for signs of inflammation around the implant abutments, and for implant mobility.

Use the Neo Screwdriver to make sure the Equator Abutment is tightened before the patient leaves the praxis.